

Certificate of Analysis

Cell Count	2.6 Million per vial
Viability	77%
CD3+	0.80%
CD19+	82.00%
CD86+	91.73%
CD40+	99.66%
HLA-DR+	99.38%
CD80+	58.90%
CD274+	53.91%
Sterility Testing	Negative for bacteria and fungi

Donor Information






Donor ID	3
Gender	Male
Age	56
Race	Caucasian
Height	unknown
Weight	unknown
ABO Type	unknown

HLA Typing

	Allele 1	Allele 2
HLA-A	02:01	02:01
HLA-B	14	27:05
HLA-C	unknown	unknown
HLA-DRB1	15:01	14

Donors are tested for the blood borne pathogens HIV-1 and 2, Hepatitis B, Hepatitis C and HTLV-1 and are negative. Cells should still be handled as if potentially infectious following biosafety level 2 procedures.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

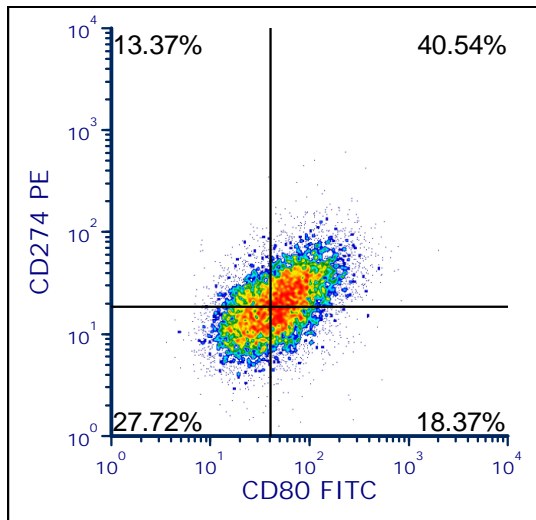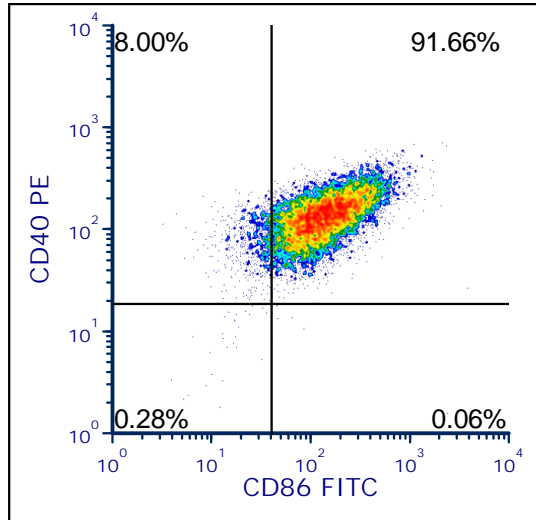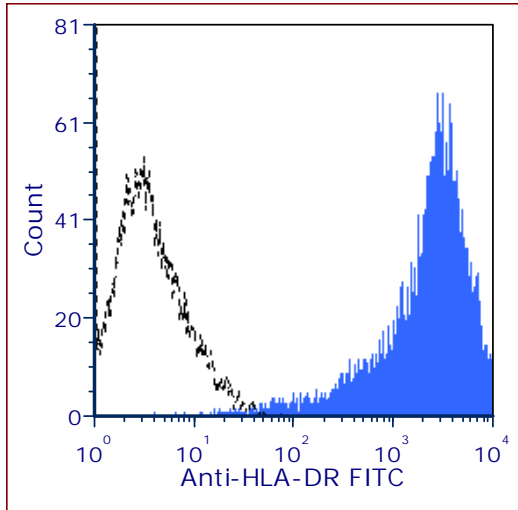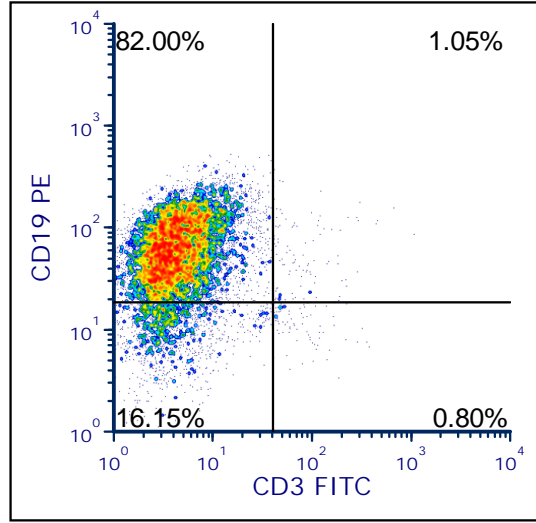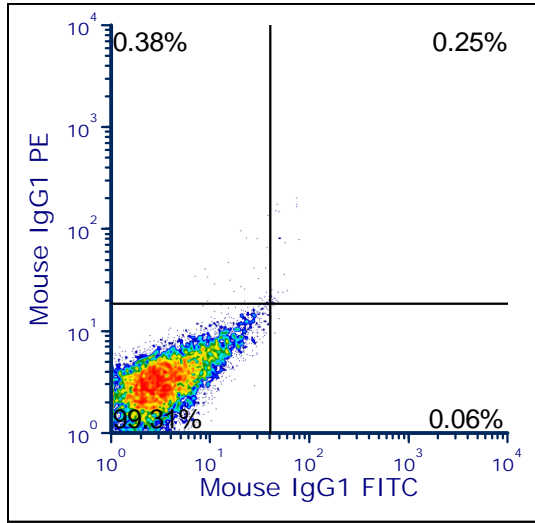

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.