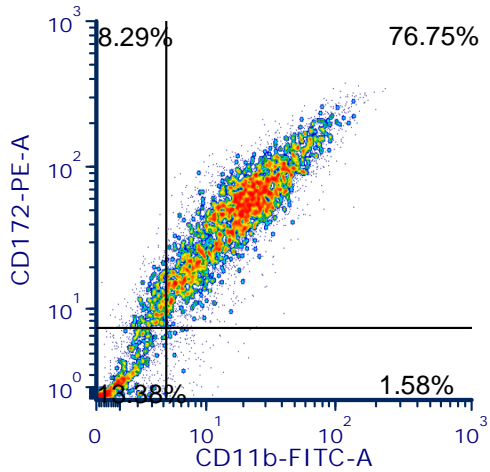
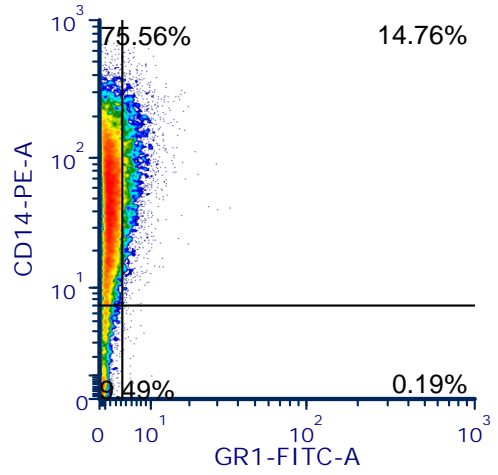
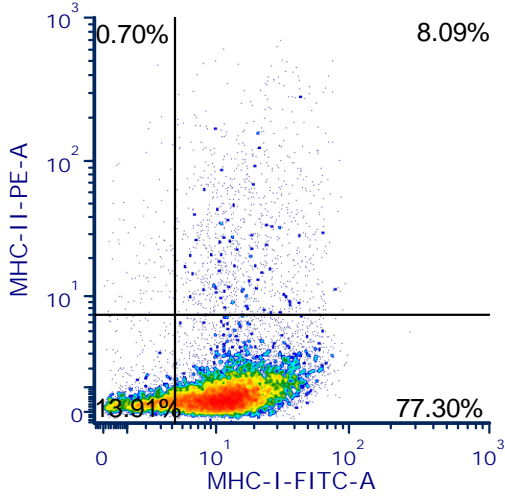
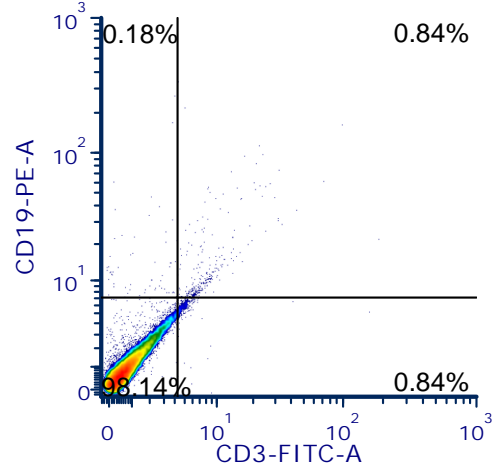
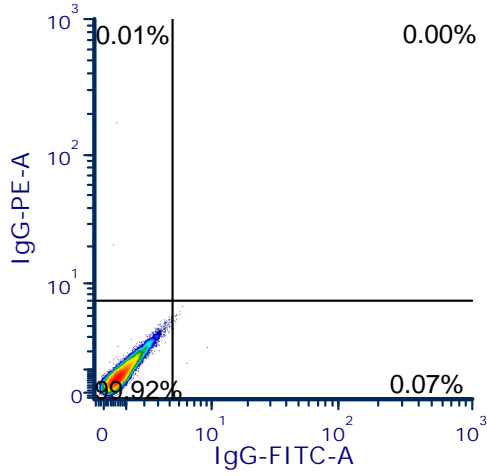

Certificate of Analysis

Cell Count	9.75 Million per vial
Viability	96%
CD3+	1.7%
CD19+	1.0%
MHC Class I	85.4%
MHC Class II	8.8%
CD14+	90.3%
GR-1+	15.0%
CD172+ CD11b+	76.7%
Sterility Testing	Negative for bacteria and fungi

Cells should still be handled as if potentially infectious following biosafety level 2 procedures.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.



FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.